

Effects of Transcranial Direct Current Stimulation (tDCS) on Operator Vigilance:

A Double-Blind, Sham-Controlled Study

E. Susan Duncan¹, Surani G. Nakkawita¹, Heather Lucas¹, Owen T. Carmichael², Marcio de Queiroz¹

1. Louisiana State University

2. Pennington Biomedical Research Center



LOUISIANA STATE UNIVERSITY



Introduction

Problem:

- Society is increasingly reliant on automation
- Monitoring such systems is essential but tedious
- Vigilance decrement in human operators creates significant safety risks¹

Proposed Solution:

- Transcranial direct current stimulation (tDCS) is safe, portable, and relatively inexpensive
- Previous work suggests anodal tDCS applied to left dorsolateral prefrontal cortex (dlPFC) can improve task vigilance^{2,3}

Methods

Design

- 21 healthy young adults completed 2 sessions
- Active or sham tDCS; order counterbalanced
- 7 or 14 days between sessions, same time/day

Task

- Computerized version of Mackworth clock test⁴
- ~8% of 3600 trials required response
- Evenly distributed across three 10-minute blocks

Stimulation


- Neuroconn DC-Stimulator Plus
- 5 x 7 cm sponge-covered rubber electrodes
 - Anode: F3 (left dlPFC)
 - Cathode: Fp2 (contralateral forehead)
- 2 mA x first 20 minutes of task

Statistics

- Linear mixed effects model (subjects = random)

Results

Performance Accuracy

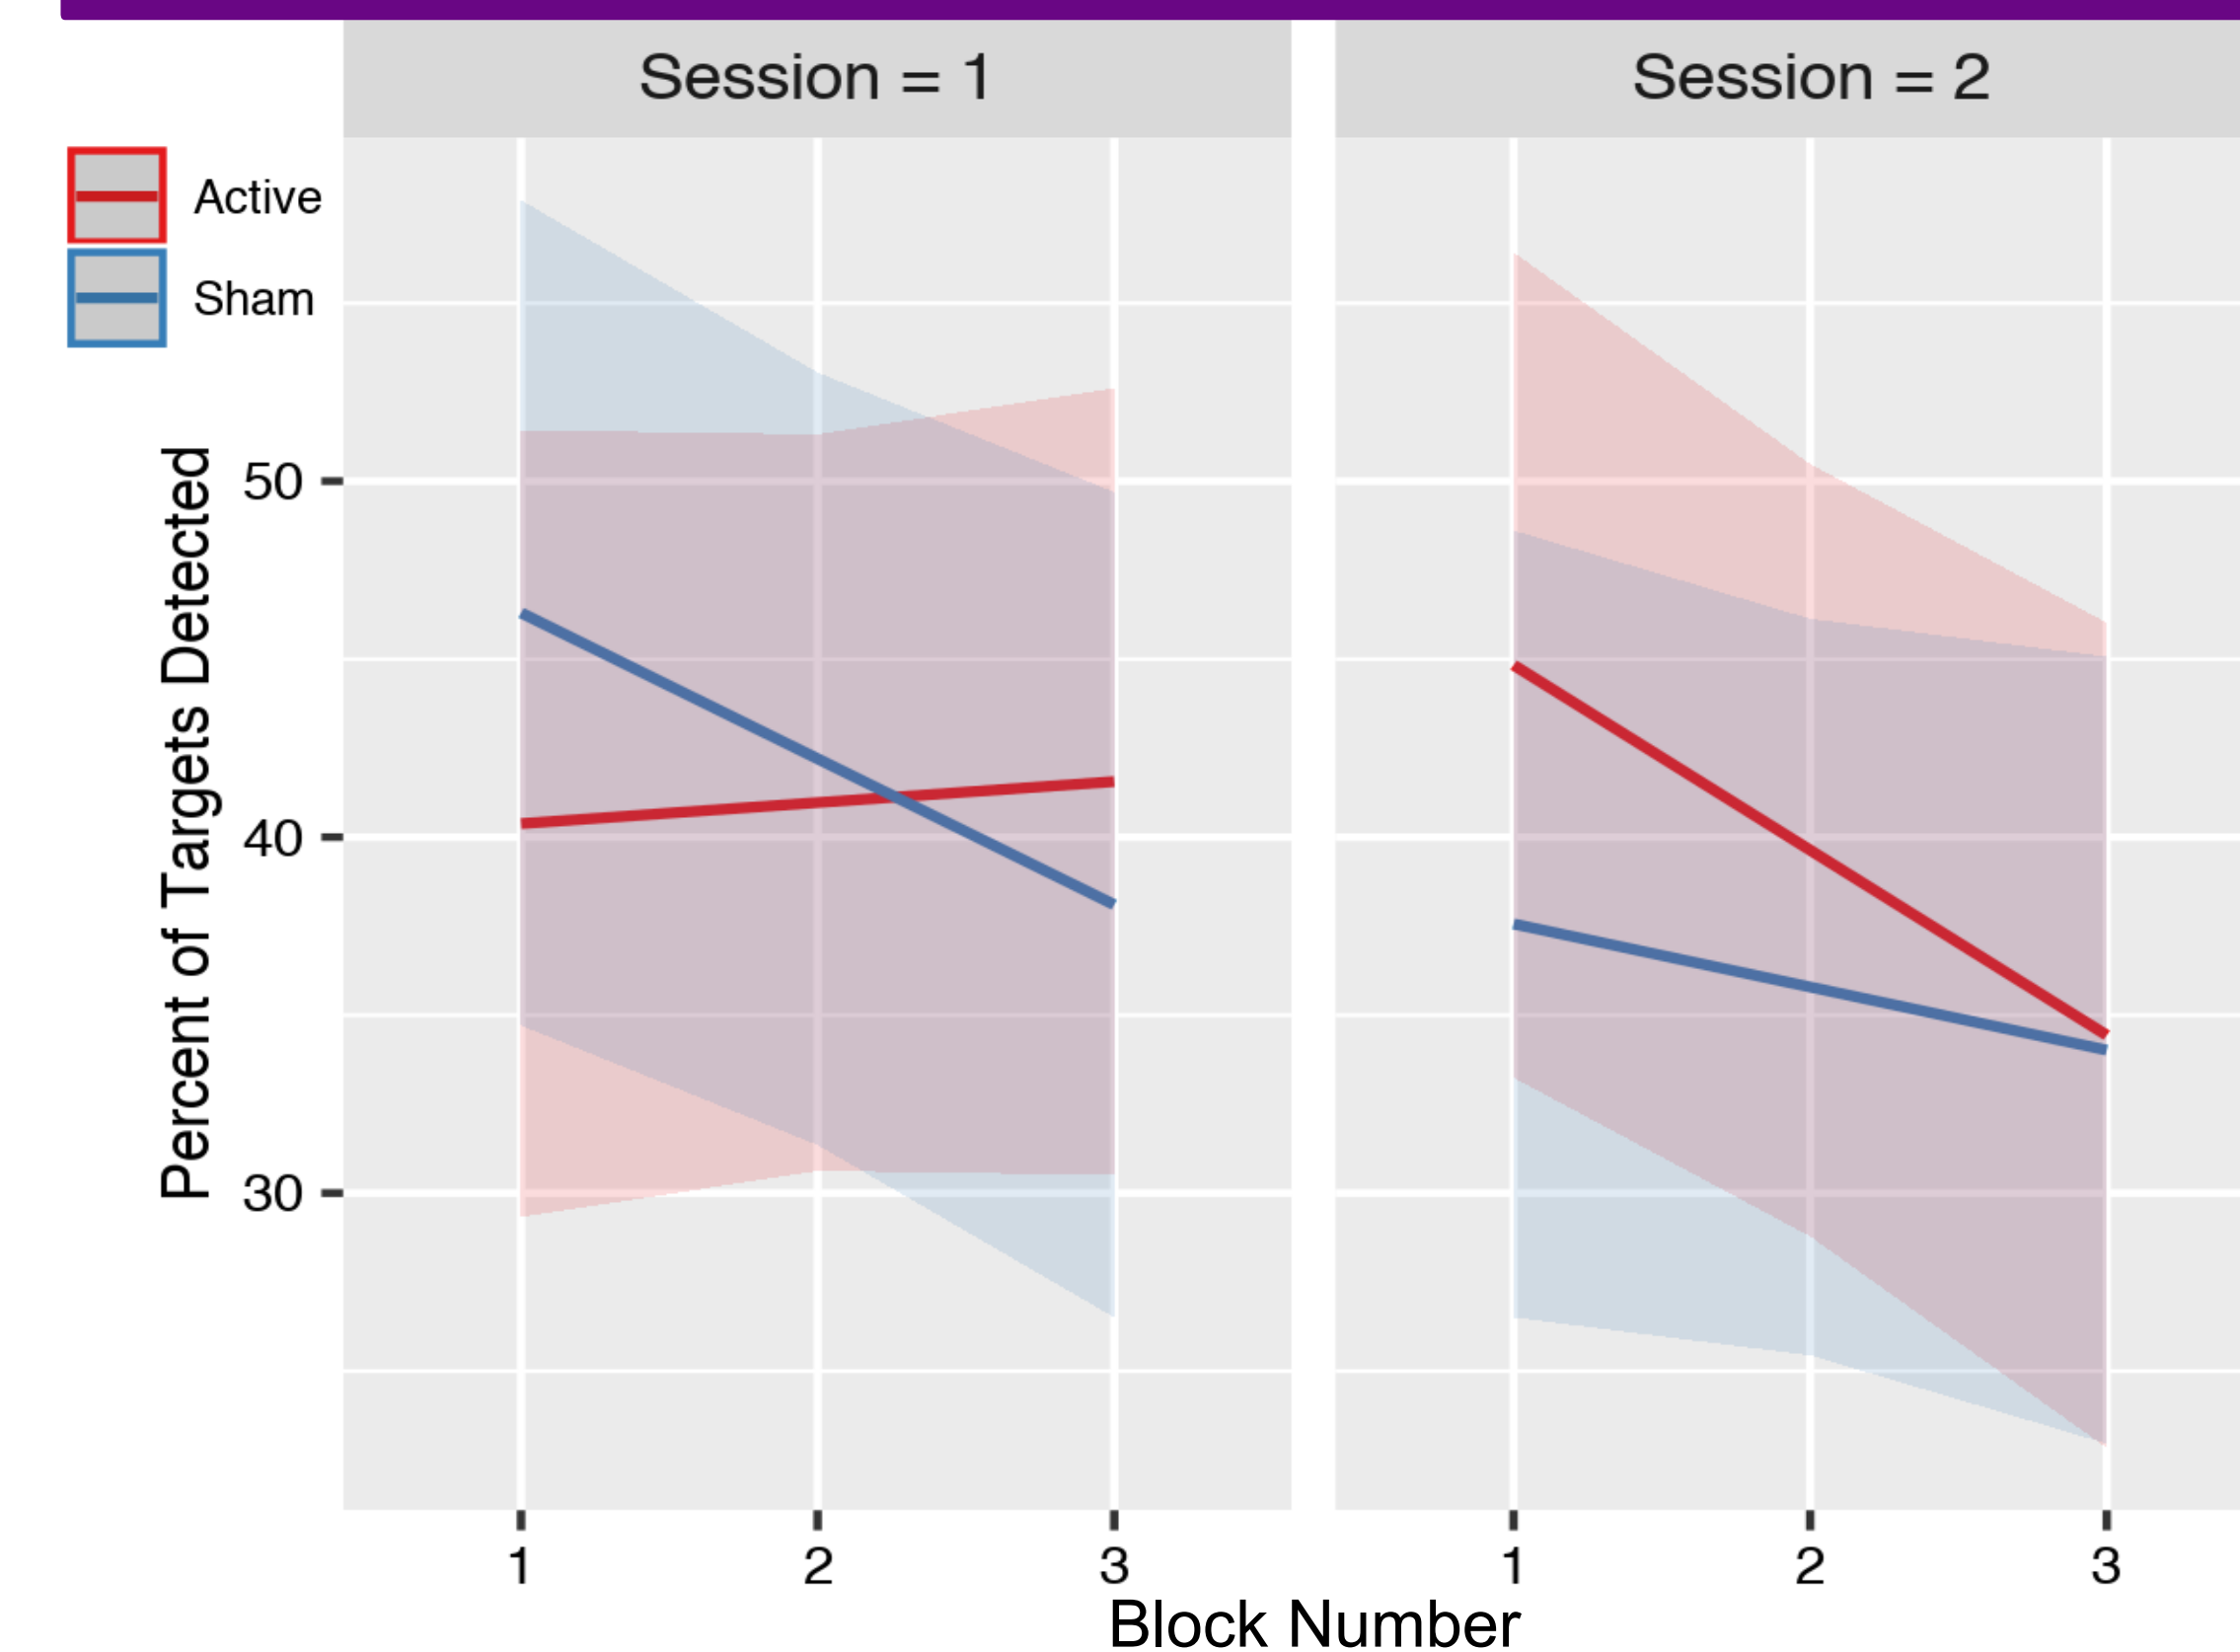

Correct Responses (True Hits)

Main Effects

- Session: $p = 0.022$
- Block: $p = 0.015$

Interaction


- Session * Block * Stimulation: $p = 0.049$

Fitted regression models for correct (above) and incorrect (below) responses.


Incorrect Responses (False Alarms)

Main Effects

- Session: $p = 0.004$
- Block: $p = 0.003$
- Stimulation: $p = 0.009$

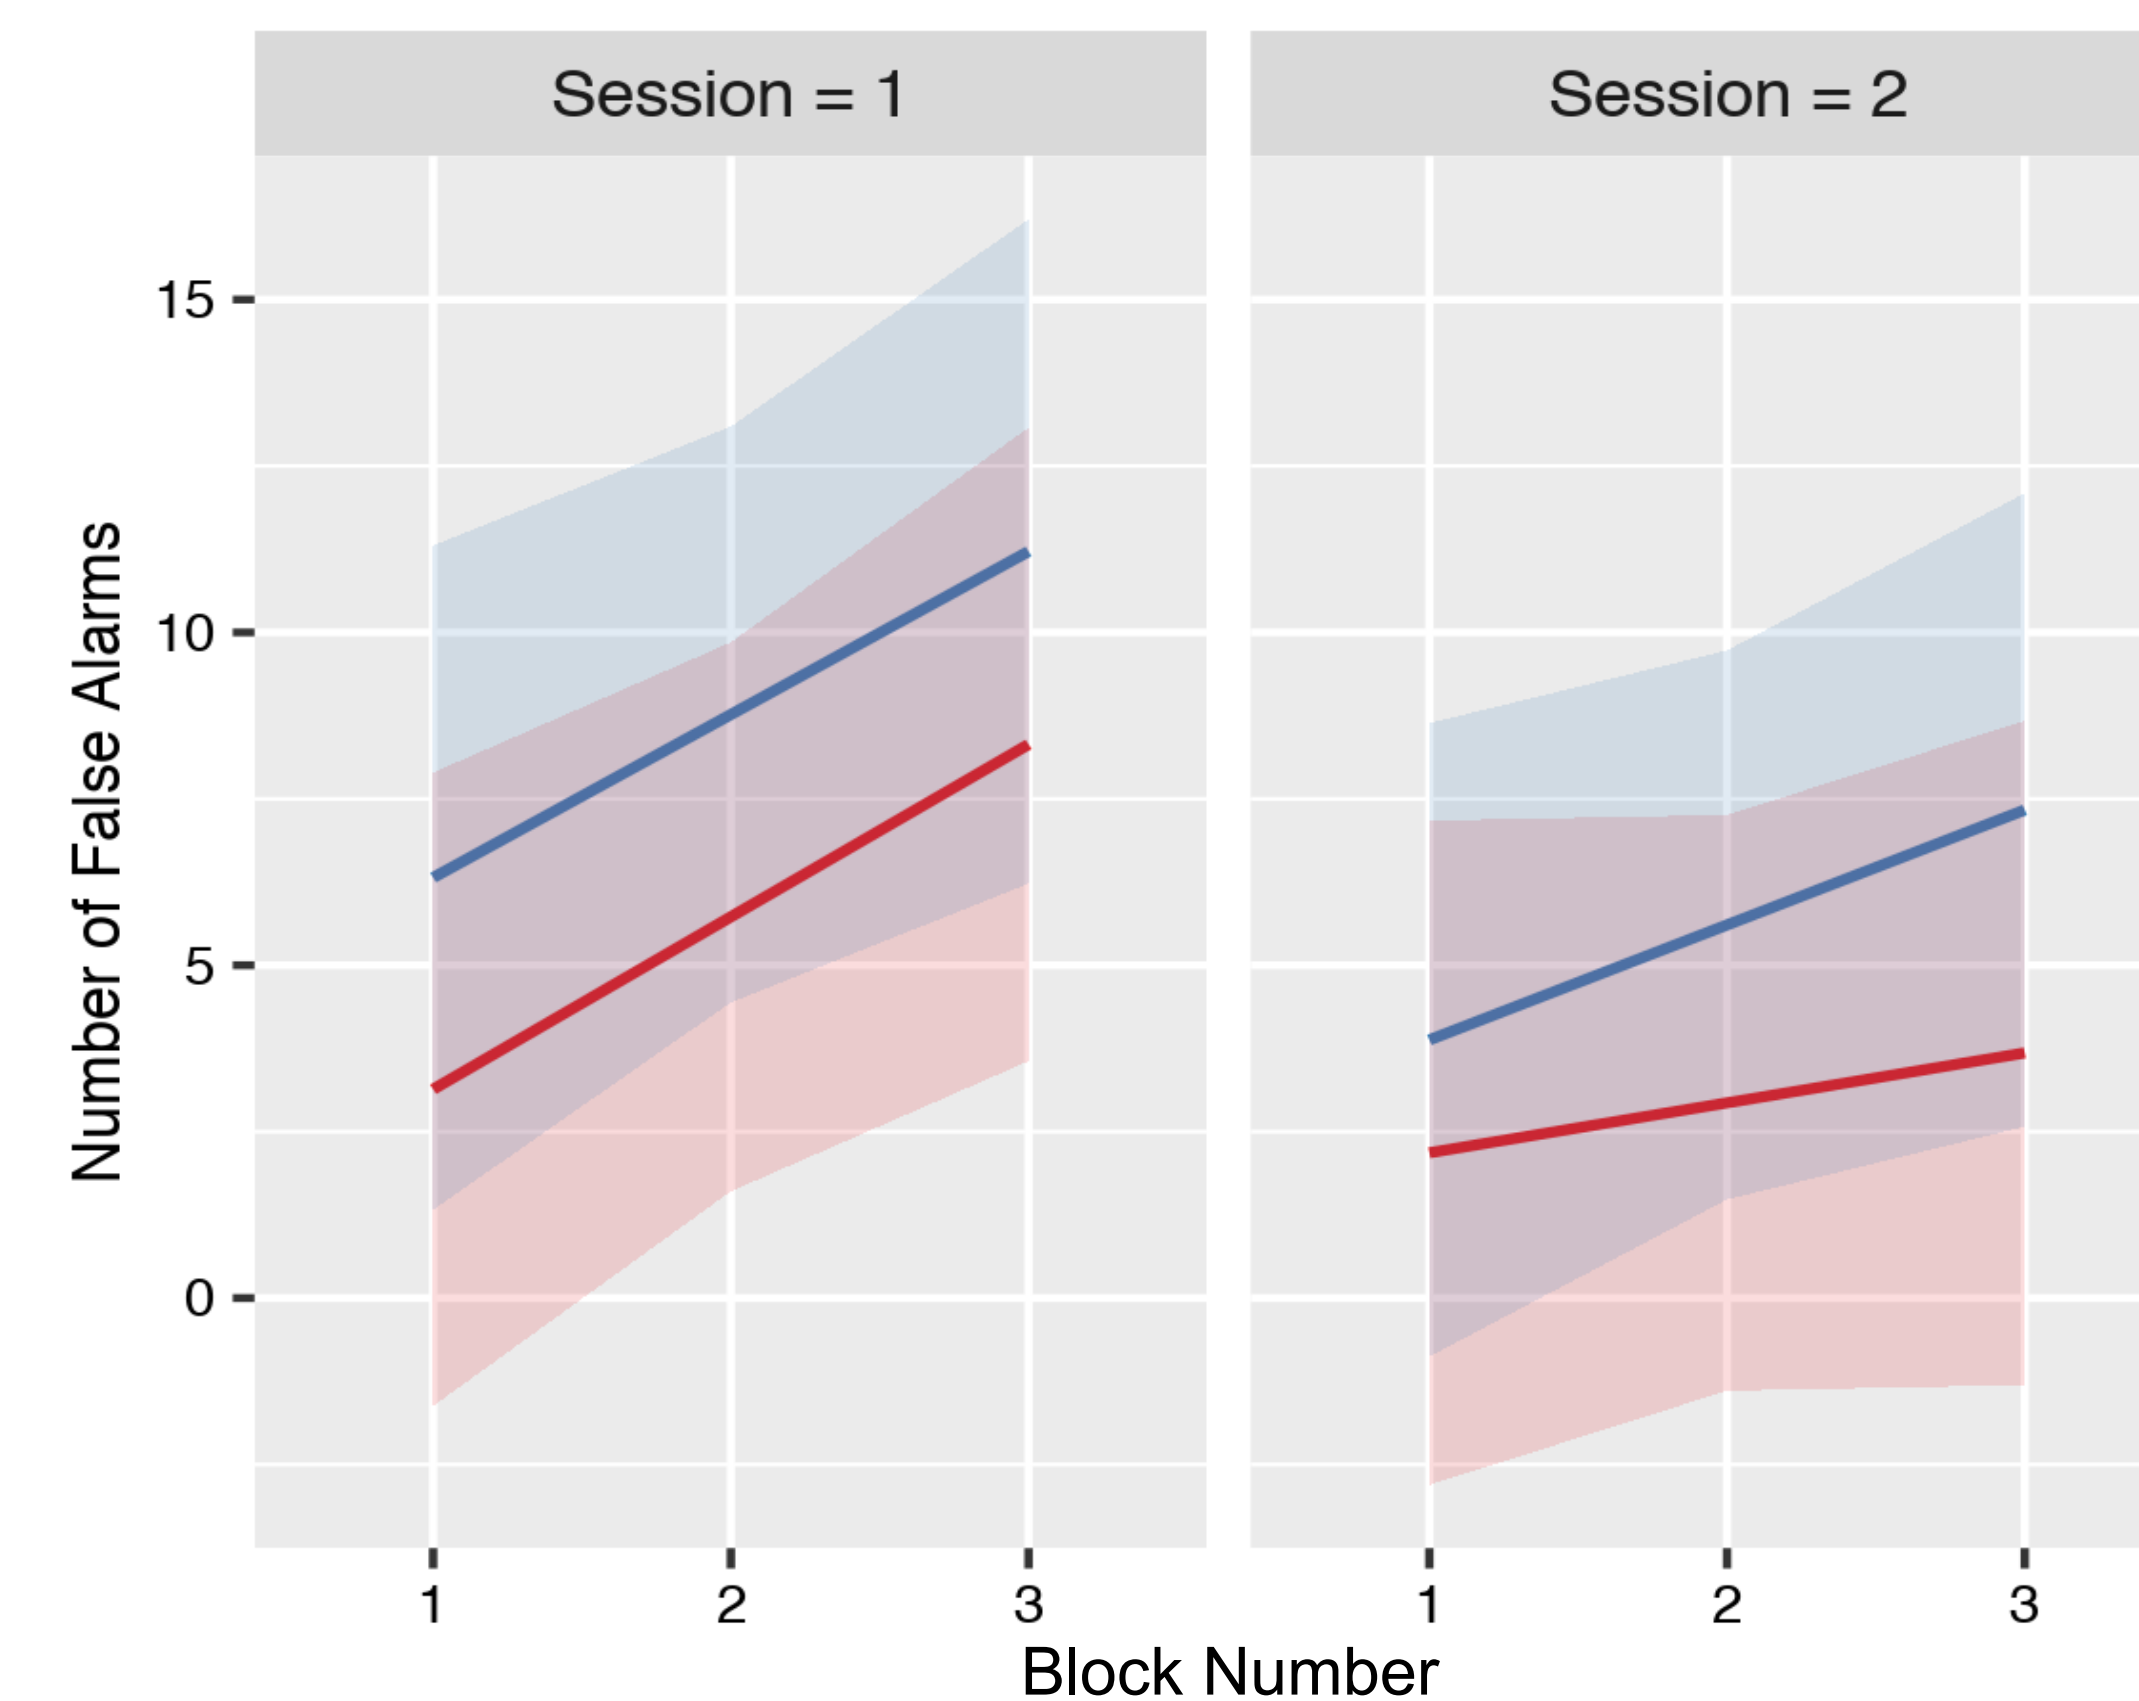


Current Modeling

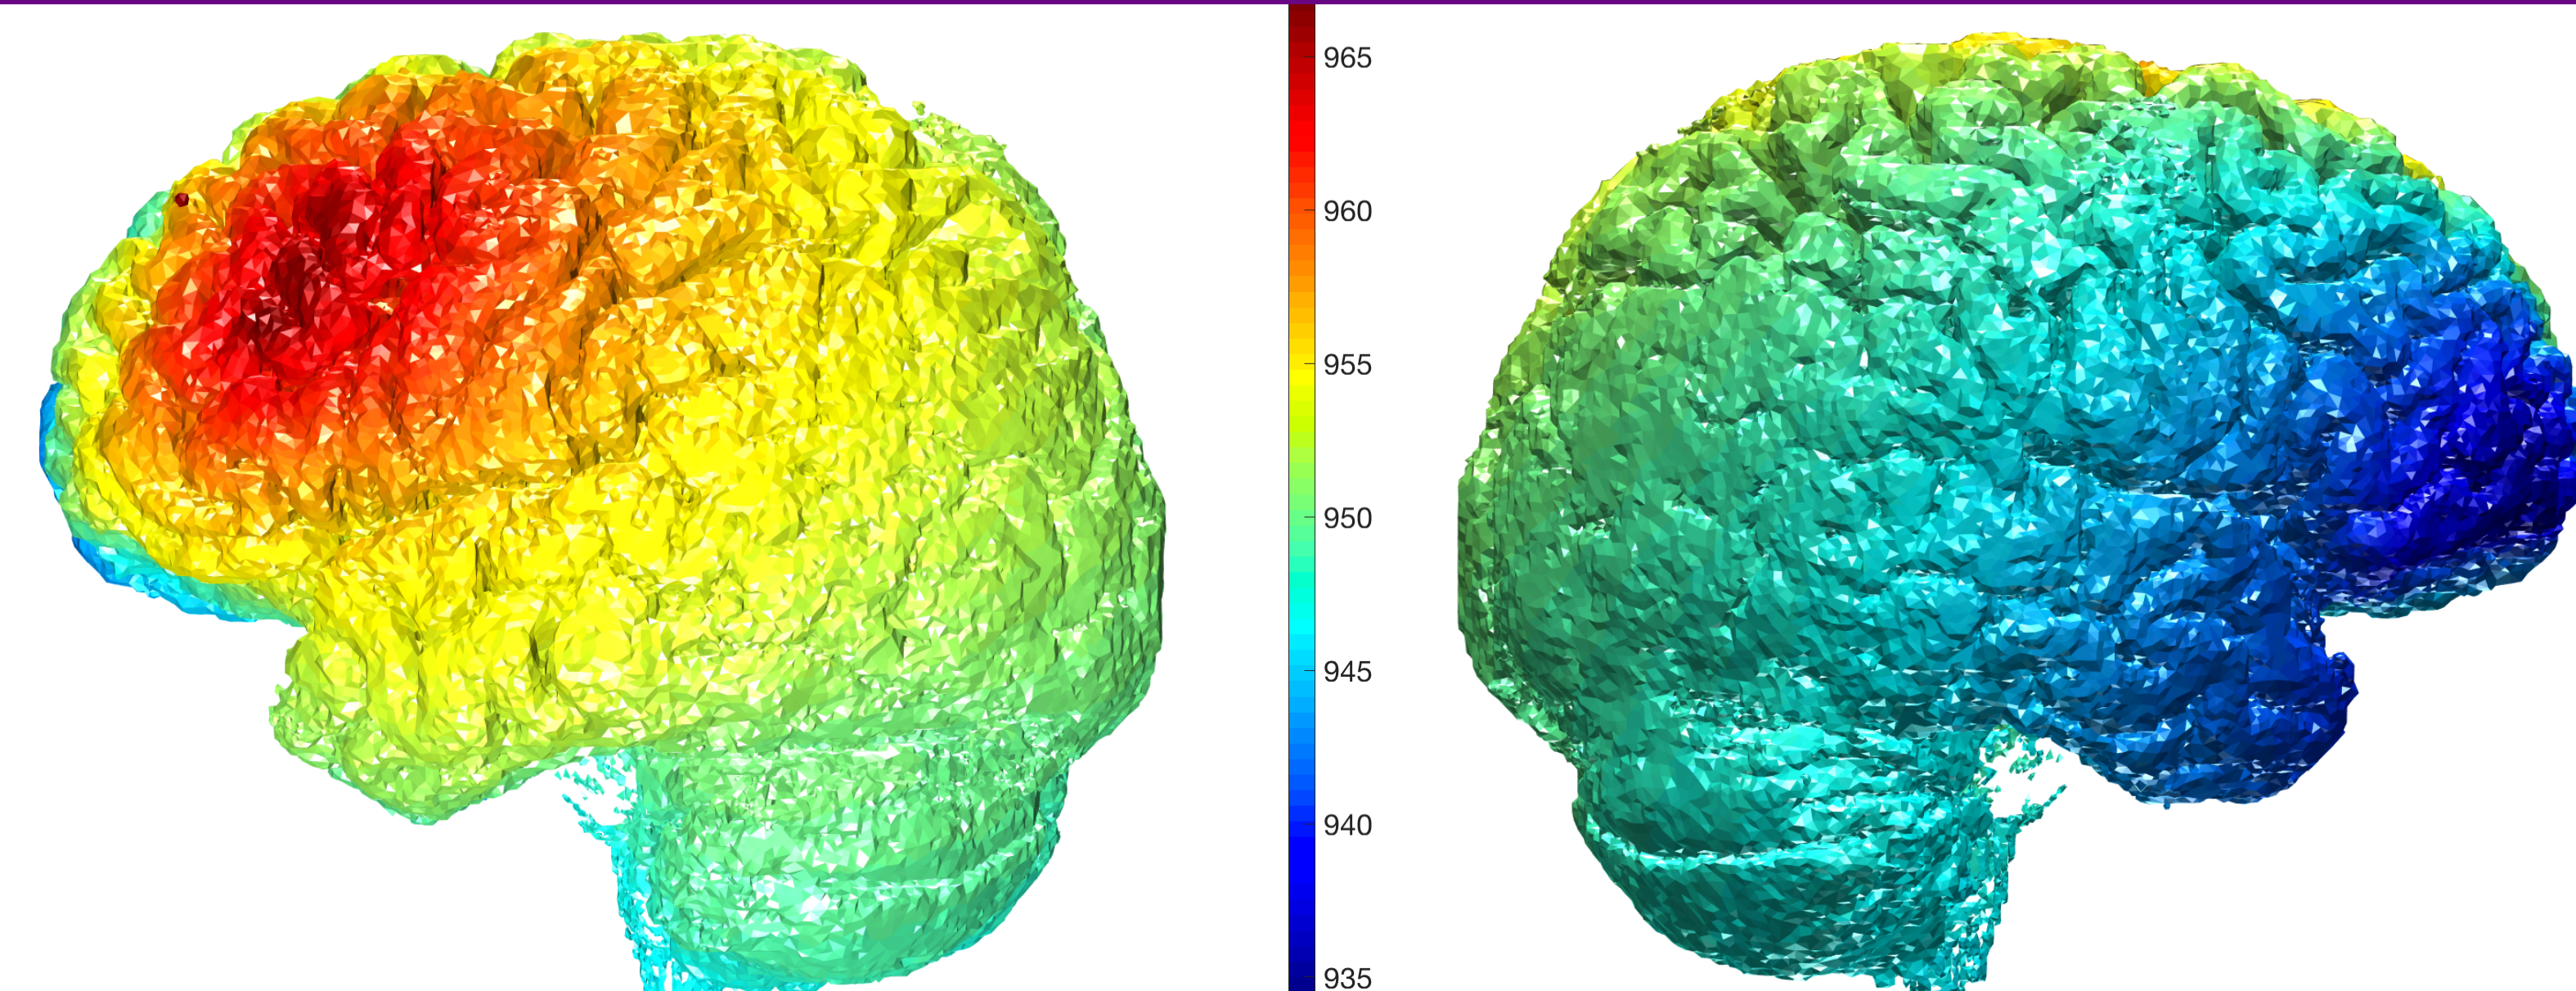


Simulated⁵ voltage measures (mV) given electrode placement and current intensity.

Individual Responses

Session 1

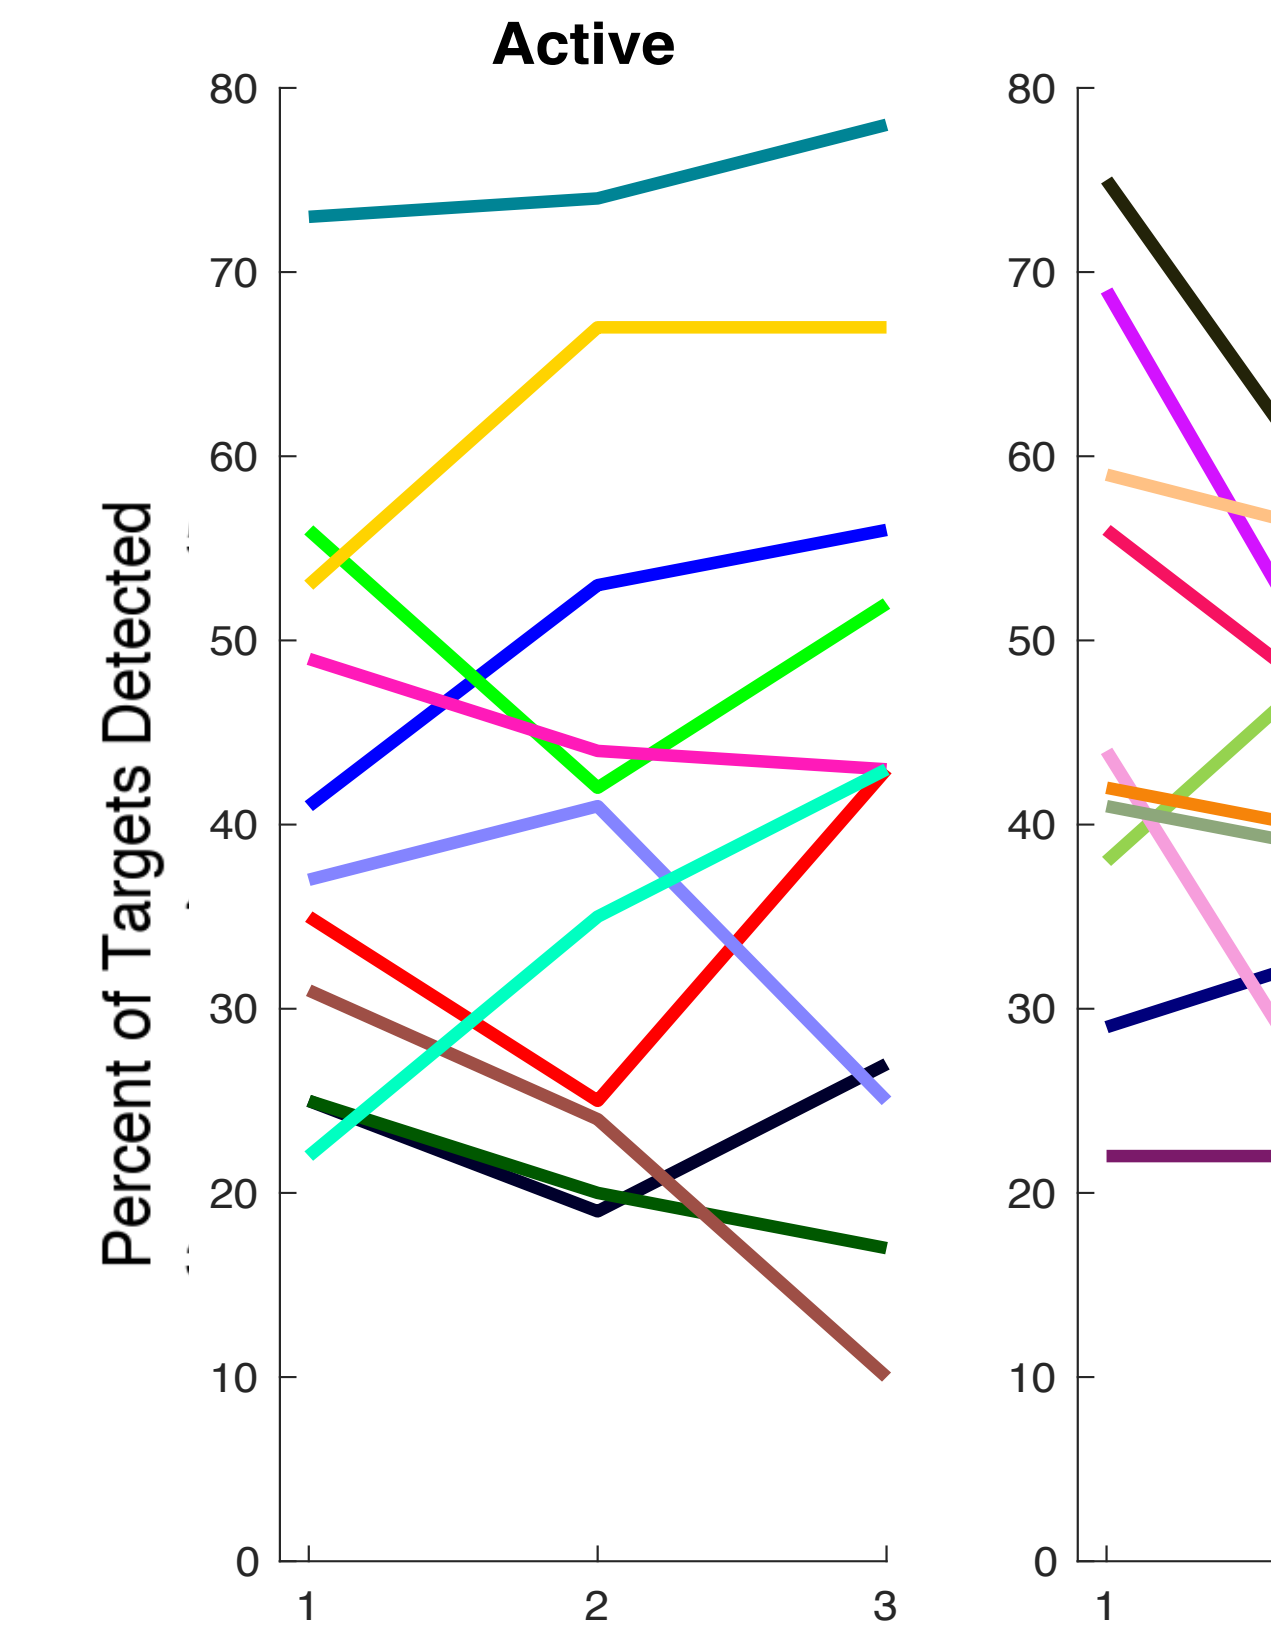

Session 2

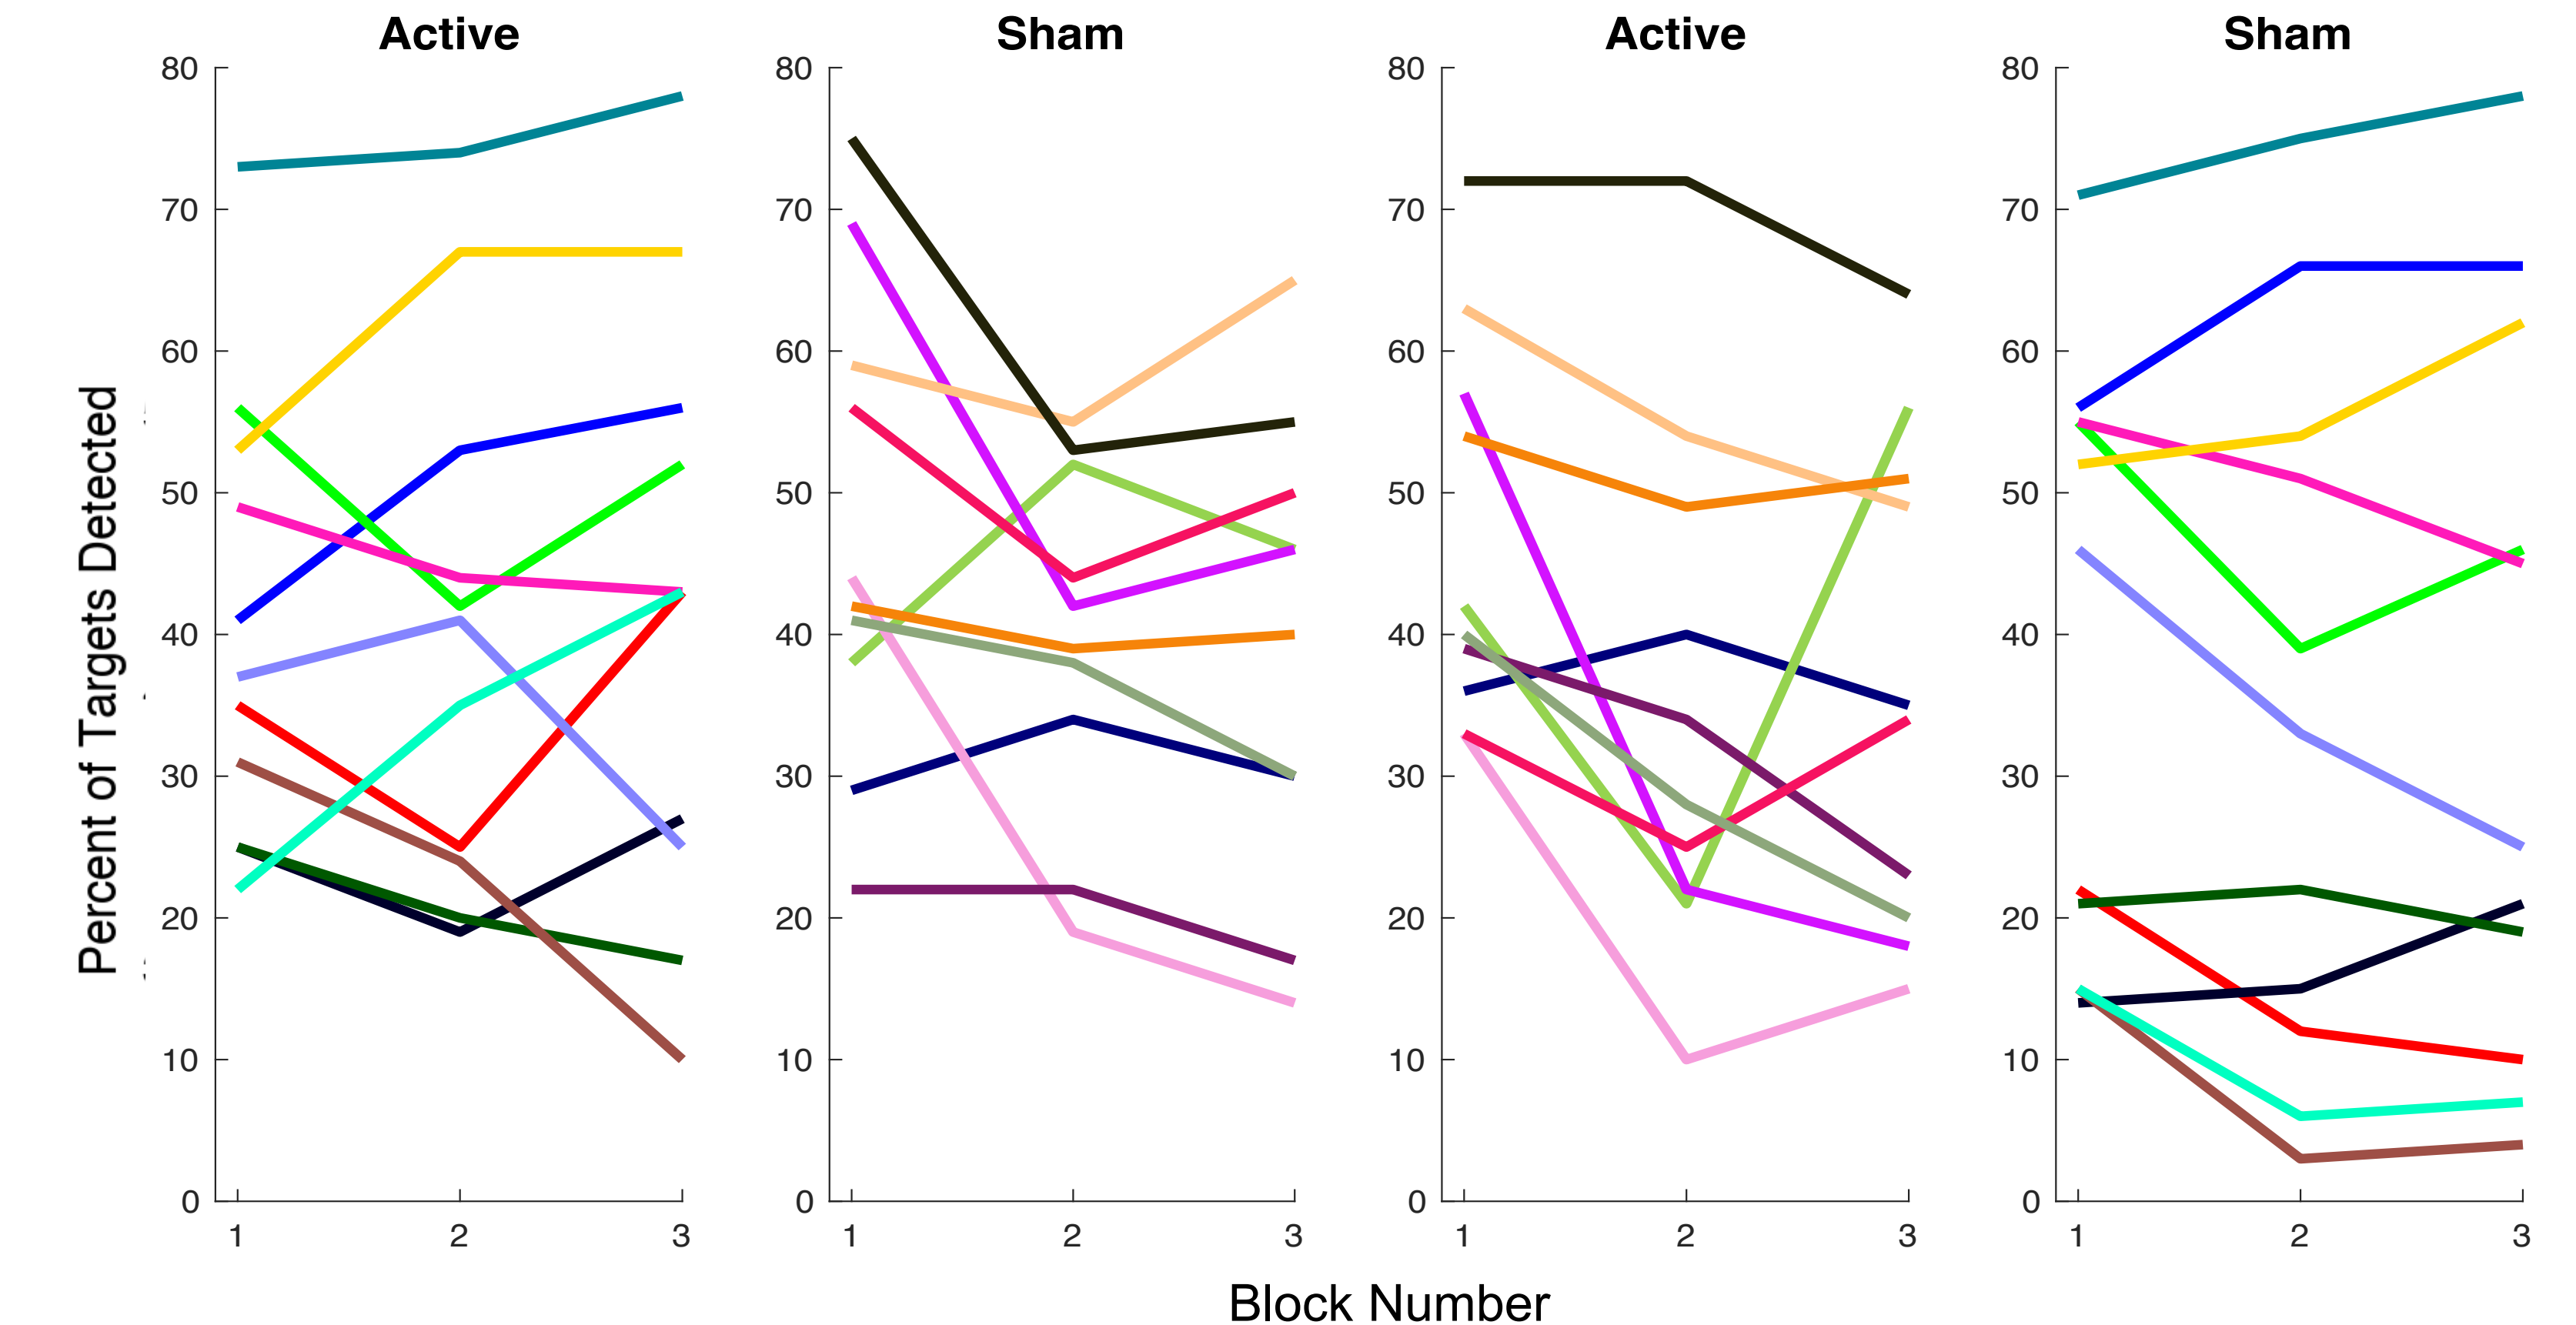

Individual performance for true hits. Color-coding conserved across plots.

Discussion

- Findings suggest future promise for enhanced operator vigilance
- Some effects likely obscured by:
 - Interaction between attention and task familiarity
 - Individual variability in tDCS response
- Modulating stimulation via real-time feedback may yield more consistent, optimal vigilance performance
 - Neural vigilance marker: Sensitive to endogenous/exogenous factors affecting attention
 - Dynamic stimulation parameters: Online adaptation of intensity/waveform based on individualized traits and states

References

1. Mosier, K. L. & Skitka, L. J. (1996). Human decision makers and automated decision aids: made for each other? In R. E. Parasuraman & M. E. Mouloua (Eds.), *Automation and human performance: Theory and applications* (pp.201-220). Hillsdale, NJ: Lawrence Erlbaum Associates, Inc.
2. Nelson, J. T., McKinley, R. A., Golob, E. J., Warm, J. S., & Parasuraman, R. (2014). Enhancing vigilance in operators with prefrontal cortex transcranial direct current stimulation (tDCS). *Neuroimage*, 85, 909-917.
3. McIntire, L. K., McKinley, R. A., Goodyear, C., & Nelson, J. (2014). A comparison of the effects of transcranial direct current stimulation and caffeine on vigilance and cognitive performance during extended wakefulness. *Brain stimulation*, 7(4), 499-507.
4. Mackworth, N. H. (1948). The breakdown of vigilance during prolonged visual search. *Quarterly journal of experimental psychology*, 1(1), 6-21.
5. Huang, Y., Datta, A., Bikson, M., & Parra, L. C. (2019). Realistic volumetric-approach to simulate transcranial electric stimulation—ROAST—a fully automated open-source pipeline. *Journal of neural engineering*, 16(5), 056006.

Acknowledgments

This work was supported by a Manship Summer Research Fellowship from the LSU College of Humanities & Social Sciences (PI Duncan) and by a grant from the Louisiana Board of Regents Research Competitiveness Subprogram (#LEQSF-(2017-20)-RD-A-03; PI Duncan).